

## VITAVM®7


	Prog. No.	Pre-drying °C	→ min.	↗ min.	↗ °C/min	Temp. °C	→ min.	VAC min.
BASE DENTINE Wash firing *	60	500	2.00	7.30	60	950	1.00	7.30
MARGIN firing	61	500	6.00	7.40	60	960	1.00	7.40
EFFECT LINER firing	62	500	6.00	8.11	55	950	1.00	8.11
1 <sup>st</sup> dentine firing	63	500	6.00	7.27	55	910	1.00	7.27
2 <sup>nd</sup> dentine firing	64	500	6.00	7.16	55	900	1.00	7.16
Fixing firing of stains	65	500	6.00	3.00	100	800	0.00	-
Glaze firing	66	500	0.00	5.00	80	900	1.00	-
Glaze firing AKZENT	67	500	4.00	5.00	80	900	1.00	-
Corrective firing with COR	68	500	4.00	6.00	55	830	1.00	6.00

\* Only for VITA In-Ceram AL for inLab

When using dental ceramics, the firing result largely depends on the individual firing procedure of the user, i.e. among other aspects on the type of furnace, the location of the temperature sensor, the firing tray as well as the size of the workpiece during the firing cycles.

Our application-technical recommendations for the firing temperatures (regardless whether they have been provided orally, in writing or in the form of practical instructions) are based on numerous own experiences and tests. The user, however, should consider this information only to provide basic values.

If surface, transparency and degree of gloss should not correspond to the firing result that is achieved under optimal conditions, the firing procedure must be adjusted correspondingly. The crucial factors for the firing procedure are not the firing temperature displayed by the furnace but the appearance and the surface condition of the firing object after the firing process.

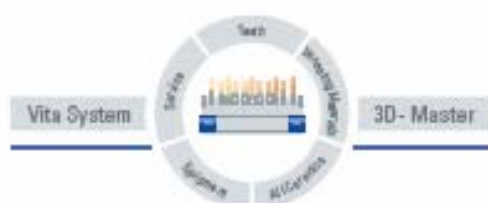

# VITA